

Location Details

Name	Vaccine Fridge
Description	
Device	S/N: 123456789
Device Model	CLT-01
Log Interval	3 minutes

Temperature

Low Temperature Alarms

Alarm Threshold	2.5°C
Alarm Delay	Immediate
Time in alarm	No Alarms

Temperature

High Temperature Alarms

Alarm Threshold	8.0°C
Alarm Delay	3 minutes
Time in alarm	46 minutes

Battery Status


Low Battery Alarms

Time in alarm	No Alarms
---------------	-----------

Connection

Offline Alarms

Alarm Delay	9 minutes
Time in alarm	1 hour, 11 minutes

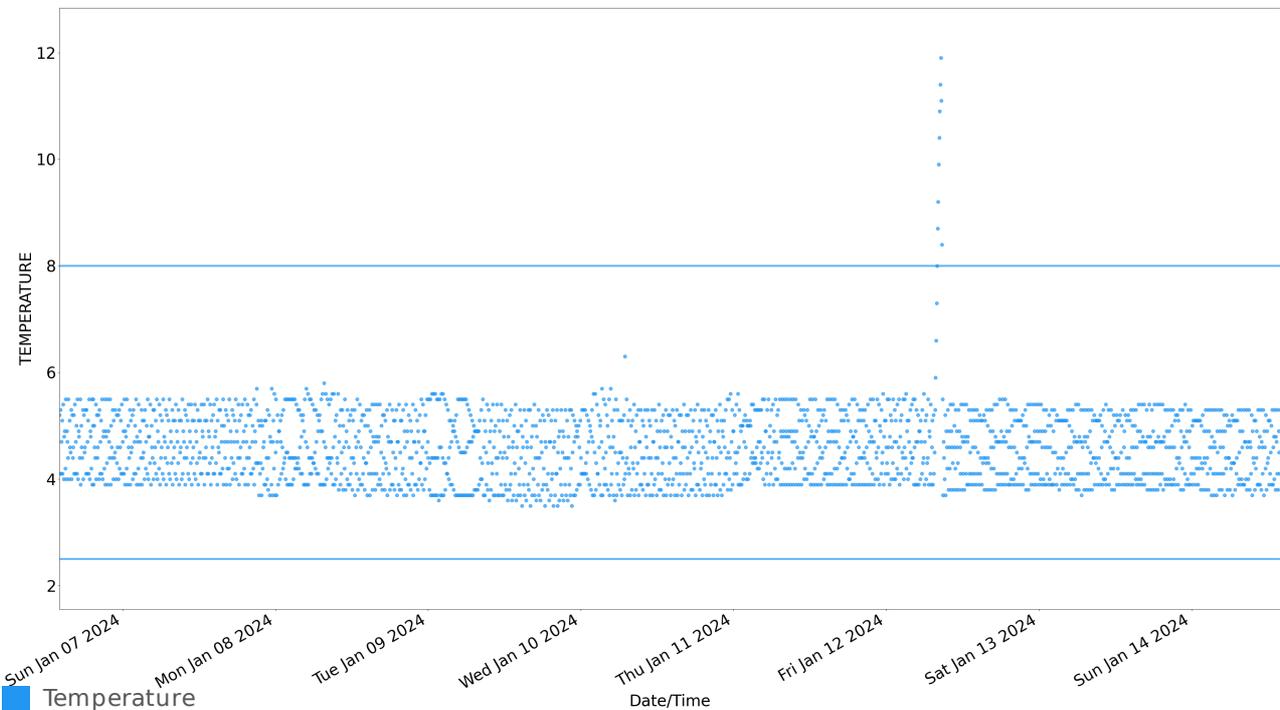

Recordings

Start date/time	End date/time	Minimum Temperature	Maximum Temperature
2024/01/07 12:00AM	2024/01/07 11:59PM	3.9°C	5.5°C
2024/01/08 12:00AM	2024/01/08 11:59PM	3.7°C	5.8°C
2024/01/09 12:00AM	2024/01/09 11:59PM	3.6°C	5.6°C
2024/01/10 12:00AM	2024/01/10 11:59PM	3.5°C	6.3°C
2024/01/11 12:00AM	2024/01/11 11:59PM	3.7°C	5.6°C
2024/01/12 12:00AM	2024/01/12 11:59PM	3.7°C	11.9°C
06:05PM			8.7°C
06:10PM			9.2°C
06:15PM			9.9°C
06:20PM			10.4°C
06:25PM			10.9°C
06:30PM			11.4°C
06:35PM			11.9°C
06:40PM			11.1°C
06:45PM			8.4°C
2024/01/13 12:00AM	2024/01/13 11:59PM	3.7°C	5.5°C
2024/01/14 12:00AM	2024/01/14 11:59PM	3.7°C	5.4°C